


SUGI et al Q68497
DERED MEDICINE MULTI-DOSE
PROBLEM 11, 2002
Bruce E. Kramer 202-293-7060
1 of 7


Fig.1

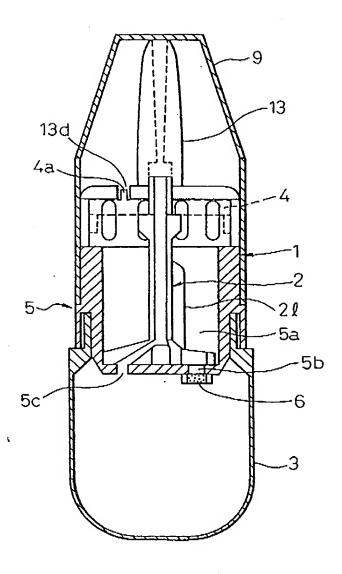

WDERED MEDICINE MULTI-DOSE
DMINISTERING DEVICE
Filed: February 11, 2002
Bruce E. Kramer 202-293-7060
2 of 7





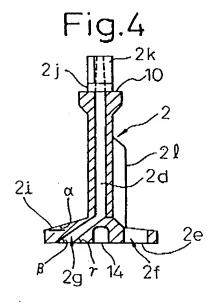

MATSUGI et al Q68497
POWDERED MEDICINE MULTI-DOSE
ADMINISTERING DEVICE
Filed: February 11, 2002
Bruce E. Kramer 202-293-7060

Fig.5




Fig.6








Fig.7




MATSUGI et al Q68497
POWDERED MEDICINE MULTI-DOSE
ADMINISTERING DEVICE
Filed: February 11, 2002
Bruce E. Kramer 202-293-7060
4 of 7

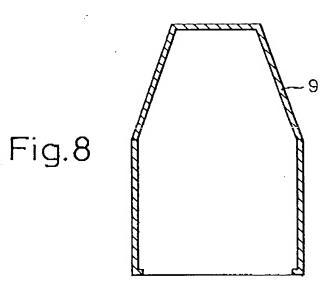


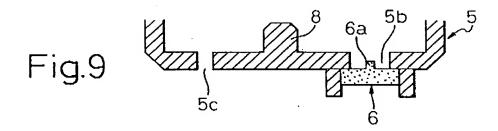




DERED MEDICINE MULTI-DOSE MINISTERING DEVICE
Filed: February 11, 2002
Bruce E. Kramer 202-293-7060
5 of 7









UGI et al Q68497 ERED MEDICINE MULTI-DOSE ADMINISTERING DEVICE Filed: February 11, 2002 Bruce E. Kramer 202-293-7060 6 of 7

Fig. 14



MATSUGI et al POWDERED M. LE MULTI-DOSE ADMINISTERIN VICE Filed: February 11, 2002
Bruce E. Kramer 202-293-7060

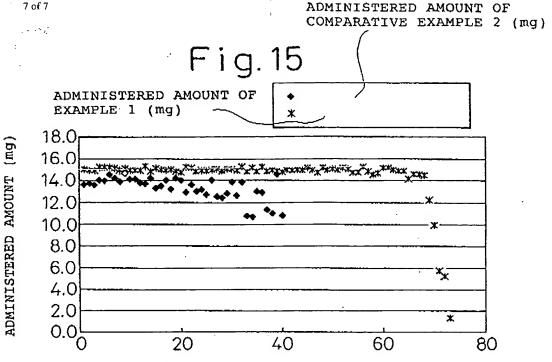

NUMBER OF TIMES OF SPRAYING

